

# PerKit™ Antibody Mc-MMAF Conjugation Kit (CM11422x1 and CM11422x3) User Reference Guide

## Contents

Important Notes & Contact Information .....	2
Kit Components.....	3
Safety Information .....	4
Labeling Chemistry.....	4
Support .....	5
Protocol.....	5
1. Lab Instrumentation Needed.....	6
2. Prepare Site and Mc-MMAF for Labeling Experiment.....	6
3. Preparation of Antibody Samples for Conjugation.....	6
4. Antibody Reduction (Step 1 in Scheme 1) .....	8
5. Purification to Remove Excess Reagent A.....	9
6. MMAF Labeling (Step 2 in Scheme 1) .....	10
7. Purification of Conjugate .....	10
Other Considerations.....	12
1. Concentration Determination for IgG Antibody (Unlabeled) .....	12
2. Concentration Determination for ADC .....	12
3. MW Calculation for ADC .....	12
4. Drug-to-Antibody Ratio (DAR) and Characterization by UV .....	13
5. Characterization of ADC by HIC HPLC .....	13
6. Characterization of ADC by SEC HPLC.....	13
7. ADC Stabilizing Buffer .....	13
8. Recommended Storage Conditions .....	14
9. Sample Submission for HPLC Analysis .....	14
Appendix: Typical Kit Performance Data (LC analysis, CellMosaic) .....	15



CellMosaic, Inc.  
10A Roessler Road  
Woburn, MA 01801  
USA

Phone: 781-463-0002  
Fax: 781-998-4694  
Email: [info@cellmosaic.com](mailto:info@cellmosaic.com)  
Website: [www.cellmosaic.com](http://www.cellmosaic.com)

---

## Important Notes & Contact Information

### READ BEFORE USING ANY RESOURCES PROVIDED HEREIN

The information provided in this document and the methods included in this package are for information purposes only. CellMosaic provides no warranty of performance or suitability for the purpose described herein. The performance of this kit in labeling may be affected by many different variables, including but not limited to the purity and complexity of the starting materials, differences in preparation techniques, operator ability, and environmental conditions.

Sample data are provided for illustration and example purposes only and represent a small dataset used to verify kit performance in the CellMosaic laboratory. Information about the chemicals and reagents used in the kit are provided as necessary.

### For Research Use Only. Not for Use in Diagnostic Procedures.

The information in this document is subject to change without notice. CellMosaic assumes no responsibility for any errors that may appear in this document. In no event shall CellMosaic be liable, whether in contract, tort, warranty, or under any statute or on any other basis for special, incidental, indirect, punitive, multiple, or consequential damages in connection with or arising from this document, including but not limited to the use thereof.


### NOTICE TO PURCHASER: LIMITED LICENSE

The purchase of this product includes a limited, non-transferable license to use this product to practice the labeling methods using the reagents solely for the purchaser's research activities. The license granted herein is personal to the original purchaser and may not be transferred to any other party outside the purchaser's company. No other right or license is conveyed or granted either expressly, by implication or by estoppel, to resell or repackage this product. Further information can be obtained by contacting:

Director of Licensing  
c/o CellMosaic, Inc.  
10-A Roessler Road, Woburn, MA 01801.  
Phone: 781-463-0002  
Fax: 781-998-4694  
E-mail: [info@cellmosaic.com](mailto:info@cellmosaic.com)

## Kit Components

This kit provides materials to conjugate 1 to 3 mg of one (CM11422x1) or three (CM11422x3) antibody samples (**IgG**) with monomethyl auristatin F (Mc-MMAF) using a maleimidocaproyl (Mc) linker.

 Upon receipt, please remove **Box 1** and store in a freezer at or below -20°C. Store **Box 2** in a refrigerator at 2-8°C.

	Name	Part #	Quantity (CM11422x1)	Quantity (CM11422x3)	Storage condition
<b>Box 1</b>	Mc-MMAF ( <b>red label</b> )	CM11010	0.11 mL	3 x 0.11 mL	-20°C
	Reagent A ( <b>blue label</b> )	CM13004	1 unit	3 units	
<b>Box 2</b>	Solution A ( <b>green label</b> )	CM01003	1.5 mL	6 mL	2-8°C
	Reducing Buffer ( <b>orange label</b> )	CM02001	4 mL	12 mL	
	Labeling Buffer ( <b>indigo label</b> )	CM02005	4 mL	12 mL	
	Storage Buffer (1 x PBS buffer) ( <b>grey label</b> )	CM02013	20 mL	60 mL	
	ADC Stabilizing PBS Buffer (5x) ( <b>pink label</b> )	CM02022	0.5 mL	1.5 mL	
	Centrifugal Filter Devices	CM03CD050A	3	9	
	Desalting Column	CM03SG10	1	3	
	Collection Tubes	CM03CT0	6	18	
	1.5 mL Centrifuge Tubes	CM03CT2	2	6	
	2.0 mL Centrifuge Tube(s)	CM03CT3	1	3	
	Hazardous Waste Bag(s)	CM03HZ1	1	3	
User Material	IgG Antibody	N/A	NOT PROVIDED (User Supplied Material, <b>1-3 mg IgG</b> needed per reaction)		

**Reaction Scale:** The protocol is optimized for conjugating 3 mg of IgG antibody. If you have less than 3 mg of IgG, use the calculations in **Steps B10, C3, D9, E2, F5, and F6** to obtain the correct volumes to be added in each step.

**Drug-to-Antibody Ratio (DAR) Optimization:** The reducing protocol is optimized for monoclonal IgG1 subtype to obtain an average 4 thiols per antibody (DAR = 4). For other IgG subtypes or polyclonal antibodies, the DAR may vary. For the best performance of the ADC and to obtain the desired DAR, you can purchase the Thiol Assay Kit with Purification ([Product #: CM90005](#)) separately and use it to perform an in-process thiol assay after the antibody reduction (**Step C5 Note Section**). The amount of reducing reagent can be adjusted based on the data to obtain your desired DAR.

## Safety Information

Warning: some of the chemicals used can be potentially hazardous and can cause injury or illness. Please read and understand the Safety Data Sheets (SDS) available at CellMosaic.com before you store, handle, or use any of the materials.

## Labeling Chemistry


The kit is designed to label any IgG antibody with monomethyl auristatin F (Mc-MMAF) using a maleimidocaproyl (Mc) linker. The user supplies the antibody. The kit includes maleimide-activated MMAF, which can be coupled directly to the antibody after reduction through alkylation in a single step (a method developed by Seattle Genetics: Sun *et al.* **2005**, *Bioconjugate Chem.* 16, 1282-1290). The product is purified to remove any unreacted drugs.



Key features of this conjugation kit:

- Offers a simple and easy way to label IgG with MMAF with minimum exposure to the toxin
- Stable linkage
- Fast and easy preparation: 6 h preparation and <2 h hands-on time
- All reagents and supplies included for preparation and purification
- Easy to control the DAR if used together with the Thiol Assay Kit with Purification ([Product #: CM90005](#))
- More than 95% conjugated products (free of unreacted drug and less than 5% unreacted antibody)

### Drug Information:

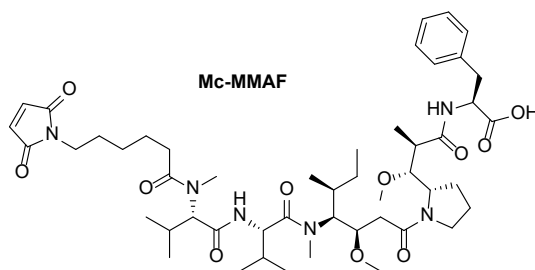

- **Name:** Monomethyl auristatin F (MMAF) with maleimidocaproyl linker
- **CAS number:** 863971-19-1
- **Chemical Formula:** C<sub>49</sub>H<sub>76</sub>N<sub>6</sub>O<sub>11</sub>
- **MW:** 925.16
- **Mechanism of action:** Inhibits cell division by blocking the polymerization of tubulin.
- **Activities:** Antioxidant, anti-inflammatory, anticancer, and insecticidal activities

- **Selected references:** 1) Doronina SO, Mendelsohn BA, Bovee TD, *et al.* Enhanced activity of monomethylauristatin F through monoclonal antibody delivery: effects of linker technology on efficacy and toxicity. *Bioconjug Chem* **2006**;17: 114–24. 2) Polson AG, *et al.* Antibody-drug conjugates for the treatment of non-Hodgkin's lymphoma: target and linker-drug selection. *Cancer Res.* **2009**;69(6):2358–2364.

#### Requirement for antibody (IgG):

1. Preferably > 90% pure by gel electrophoresis
2. Total amount: 1-3 mg protein content as measured by UV. Note: the accuracy of your protein amount is the single most important factor to obtaining an optimized DAR. Please refer to the section Other Considerations in this manual to measure the protein amount.


## Support

A customer can request a recommendation for the conjugation if the IgG has a special feature or less than 1 mg of IgG to be labeled. CellMosaic provides other accessory tools, such as buffers, standards, and reagents for ADC research. CellMosaic also provides fee-based support services to customers who need help analyzing the final conjugates by HPLC and determining the DAR.

## Protocol



Cap and briefly spin the tubes before opening

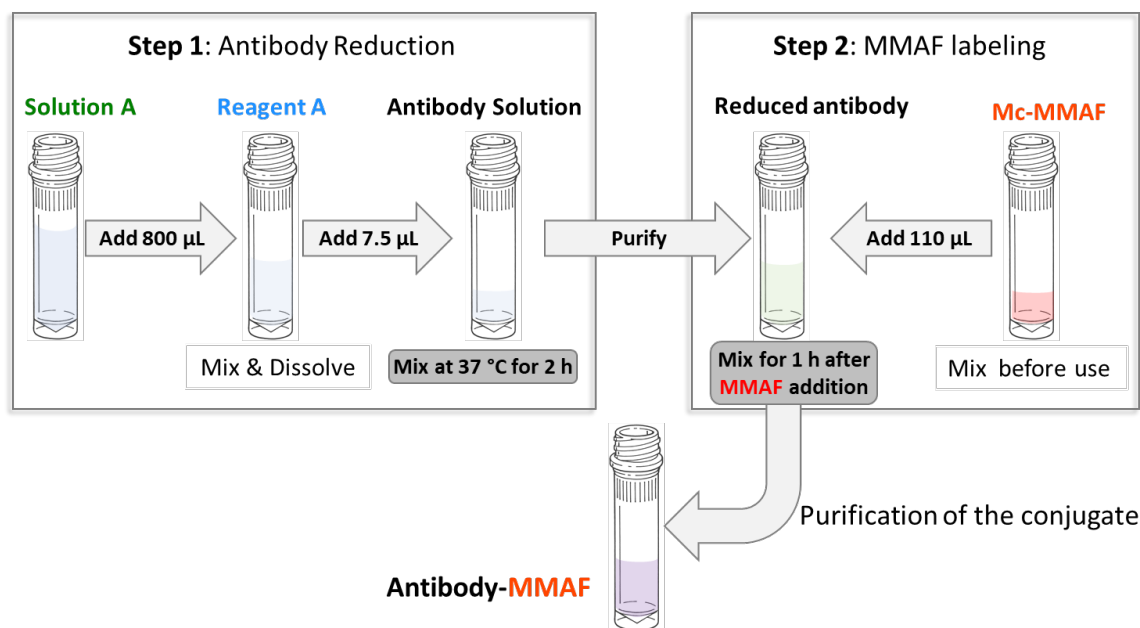

**Scheme 1.** Schematic diagram of the workflow for preparing antibody-MMAF conjugates starting with 3 mg of IgG (volume of reagents varies if the amount of IgG is < 3 mg).

## 1. Lab Instrumentation Needed

- Vortex mixer, centrifuge (preferably refrigerated, 14,000 g capable), mini-centrifuge.
- Pipettes and tips
- Timer
- Incubator or shaker set at 37°C and at RT
- Chemical hood
- Support stand, lab frame, or any support rod for desalting column
- Flask
- Personal protection equipment (lab coat, safety glasses, and chemical resistant nitrile gloves)

## 2. Prepare Site and Mc-MMAF for Labeling Experiment

**Note:** Mc-MMAF is very hydrophobic. Antibody-drug conjugates with average 2-4 MMAF per antibody tend to aggregate and precipitate out from the solution over time. It is recommended that the labeling experiment be planned right before your other experiments. If not possible, then please use the supplied ADC Stabilizing PBS Buffer to store under recommended conditions.

Ensure you use personal protection equipment (lab coat, safety glasses, and chemical resistant nitrile gloves) while handling Mc-MMAF. Locate a clean space inside a chemical hood.

**A1.** Remove **Box 1** containing **Mc-MMAF** (red label) and **Reagent A** (blue label) from the -20°C freezer and warm to RT before opening the bag.

**A2.** Remove **Box 2** from the refrigerator. Take the hazardous waste bag and place it inside the chemical hood for solid waste disposal. Bring the rest of the items to a lab bench.

**A3.** Check if the frozen liquid is thawed inside the **Mc-MMAF** tube. Briefly mix & spin the centrifuge tube containing **Mc-MMAF**. Place the **Mc-MMAF** tube in a tube holder inside a chemical hood and wait until the antibody is ready for conjugation.

**Tip for opening centrifuge tubes after mixing:** Always spin the tubes to ensure no liquid is in the cap.

**A4.** Set the temperature of the incubator or shaker to 37°C.

## 3. Preparation of Antibody Samples for Conjugation

Items needed: Filter Devices (CM03CD050A), Collection Tube (CM03CT0), Reducing Buffer (CM02001, Orange label), 1.5 mL Centrifuge Tube (CM03CT2), Clean Centrifuge Tubes (not provided in the kit).

Total amount of antibody used for the conjugation is 3 mg per reaction (protein content measured by UV). The protocol is optimized for the monoclonal IgG1 subtype antibody to obtain 4 drugs per antibody.

**Reaction Scale:** If you have less than 3 mg of antibody, use the calculations in **Steps B10, C3, D9, E2, F5, and F6** to obtain the correct volumes to be added in each step.

**DAR Optimization:** If you have non-IgG1 subtype or polyclonal antibody and would like to adjust the loading, follow **Step C5 Note Section** for optimization.

**B1.** Insert the **Filter Device** into one of the provided collection tubes (micro-centrifuge tube with the cap attached). Perform the step based on the following conditions.

- ✓ If your antibody is supplied as a lyophilized solid, dissolve the antibody in 500  $\mu\text{L}$  of **deionized water** and then transfer the entire contents to the **Filter Device**.
- ✓ If your antibody is supplied in < 500  $\mu\text{L}$  buffer, transfer your antibody sample to the **Filter Device** directly. Add **Reducing Buffer** to make up the total volume to 500  $\mu\text{L}$  and cap it.
- ✓ If the volume of your antibody sample is between 500 and 1000  $\mu\text{L}$ , divide the volume into two **Centrifugal Filter Devices** and add the antibody sample to the filter device. Add **Reducing Buffer** to make up the total volume to 500  $\mu\text{L}$  in each device and cap them.
- ✓ If the volume of your antibody sample is >1000  $\mu\text{L}$ , add up to 500  $\mu\text{L}$  of sample to the two **Filter Devices** and cap them. Repeat **Steps B1-B4** until all of the antibody sample is transferred into the **Filter Device**. Move on to **Step B5**. Add **Reducing Buffer** to make up the total volume to 500  $\mu\text{L}$  in each device for the last refill.

**B2.** Place the capped **Filter Device** into the centrifuge rotor, aligning the cap strap toward the center of the rotor; counterbalance with a similar device.

**B3.** Spin the **Filter Device** at 14,000 x g for 8 minutes (preferably cooled to 4°C) to concentrate to < 100  $\mu\text{L}$  (Spin time depends on many factors. The typical spin time for a 500  $\mu\text{L}$  sample is approximately 8 to 20 minutes. The typical volume is ~40  $\mu\text{L}$  after spinning for 8 minutes on an Eppendorf 5417R at 4°C).

**B4.** Remove the assembled device from the centrifuge and separate the **Filter Device** from the collection tube. Transfer the filtrate from the collection tube to a clean centrifuge tube (not provided). **Save the filtrate until the experiments are done.**

**B5.** Insert the **Filter Device** back into the collection tube. Add 400-450  $\mu\text{L}$  of **Reducing Buffer** to make up the total volume to 500  $\mu\text{L}$ . Next, place the capped **Filter Device** into the centrifuge rotor, aligning the cap strap toward the center of the rotor; counterbalance with a similar device. Spin the device at 14,000 x g to concentrate to < 100  $\mu\text{L}$ . Remove the assembled device from the centrifuge and separate the **Filter Device** from the collection tube. Transfer the filtrate from the collection tube to a clean centrifuge tube (not provided). **Save the filtrate until the experiments are done.**

**B6.** Repeat **Step B5** two more times.

**B7.** Transfer the concentrated sample from the **Filter Device** to a 1.5 mL micro-centrifuge tube (use the pipetman to measure the approximate volume of the concentrated sample).

**B8.** Add 20-100  $\mu\text{L}$  of **Reducing Buffer** to the **Filter Device** to rinse (actual volume of **Reducing Buffer** added will depend upon the calculated total volume in **Step B10**). Stir it gently with a pipet tip, then transfer the entire contents to the 1.5 mL micro-centrifuge tube from **Step B7**.

**B9.** Repeat **Step B8** once.

**B10.** Add **Reducing Buffer** to the 1.5 mL micro-centrifuge tube from **Step B9** to make up the total volume of the sample to  **$300 \pm 5 \mu\text{L}$**  and cap it.

**Calculation 1 for Less Antibody (Ab):**

$$\text{Total volume of the antibody in Step B10 } (\mu\text{L}) = \text{Ab in mg} \times 100$$

**B11.** Vortex the combined antibody sample for 30 seconds and then spin down.

#### 4. Antibody Reduction (Step 1 in Scheme 1)

Items needed: Reagent A (CM13004, blue label), Solution A (CM01003, green label), Antibody Solution from **Step B11**, Ice Bath.

**C1.** Spin the centrifuge tube containing **Reagent A** (blue label).

**C2.** Spin **Solution A** (green label) before opening it. Add 800  $\mu\text{L}$  of **Solution A** to the tube with **Reagent A** from **Step C1**. Vortex for 30 seconds to 1 minute to dissolve the reagent and then spin.

**C3.** Add **7.5  $\mu\text{L}$**  of **Reagent A solution** from **Step C2** to the centrifuge tube containing antibody from **Step B11** (Discard any unused **Reagent A** as hazardous chemical waste **after completion of all experiments**).

**Calculation 2 for Less Antibody (Ab):**

$$\text{Volume of Reagent A solution to be transferred in Step C3 } (\mu\text{L}) = \text{Ab in mg} \times 2.5$$

**C4.** Vortex the solution for 30 seconds, and then spin to ensure no liquid is in the cap. Mix at  $37^\circ\text{C}$  for 2 h.

**Tip for mixing:** You can use a nutator, a shaker, a vortex, or an incubator shaker for mixing. If you are using end to end nutating, make sure the tube from **step C4** is securely capped. If you don't have any of this equipment, you can let the tube sit on the bench with manual mixing by pipetting every 20 minutes.

**C5.** Cool the reduced antibody solution to approximately  $4^\circ\text{C}$  by placing the tube on ice or keeping it inside a refrigerator at  $2-8^\circ\text{C}$  for 5 minutes.

**Note: Optimization of Thiol Content for non-IgG1 Subtype Antibody or Polyclonal Antibody**



For the monoclonal IgG1 subtype, the average free thiol groups per antibody is 4 after reduction. If you have a polyclonal or other IgG subtype, you can purchase the Thiol Assay Kit with Purification ([Product Number: CM90005](#)) separately from CellMosaic to measure the free thiols while letting the reducing solution sit at 4°C in **Step C5**. Use 6 µL antibody solution from **Step C5** and follow the protocol of CM90005. To calculate the number of thiols, please use the antibody concentration of 13 µM.

The assay will take 30 minutes. The number of thiols per antibody (**n**) is satisfactory within 3-5. If **n** is lower (i.e., <3.0), you can add additional Reagent A solution from **Step C2** based on the following calculation. Repeat **Step C4**, but mixing at 37°C for 30 minutes will be sufficient, and then cool the antibody reducing solution to approximately 4°C for 5 minutes before moving to the next purification step.

**Calculation for Additional Reagent A Solution for Targeting Total 4 Thiols per Antibody:**

$$\begin{aligned} & \text{Volume of Additional Reagent A solution to be transferred from Step C2 } (\mu\text{L}) \\ &= \text{Ab in mg} \times 2.5 \times \left(\frac{4 - n}{n}\right) \end{aligned}$$

## 5. Purification to Remove Excess Reagent A



The following steps are to be performed without any break. Reduced thiols tend to oxidize quickly. Make sure **step A3** is completed prior to the following steps. Work quickly through **steps D6-D8**.

**Items needed:** [Filter Device \(CM03CD050A\)](#), [Collection Tube \(CM03CT0\)](#), [Labeling Buffer \(CM02005, indigo label\)](#), [Clean Centrifuge Tubes \(not provided in the kit\)](#), [Antibody Solution from Step C5](#).

**D1.** Insert the **Filter Device** into one of the provided collection tubes (micro-centrifuge tube with the cap attached). Transfer the reduced antibody solution from **Step C5** into the **Filter Device** directly. Wash the centrifuge tube once with 200 µL **Labeling Buffer**, transfer the solution to the **Filter Device** (total volume 500 µL), and cap it. Place the capped **Filter Device** into the centrifuge rotor, aligning the cap strap toward the center of the rotor; counterbalance with a similar device.

**D2.** Spin the **Filter Device** at 14,000 x g for 8 minutes (preferably cooled to 4°C) to concentrate to < 100 µL.

**D3.** Remove the assembled device from the centrifuge and separate the **Filter Device** from the collection tube. Transfer the filtrate from the collection tube to a clean centrifuge tube (not provided). **Save the filtrate until the experiments are done.**

**D4.** Insert the **Filter Device** back into the collection tube. Add 400-450 µL of **Labeling Buffer** to make up the total volume to 500 µL. Next, place the capped **Filter Device** into the centrifuge rotor, aligning the cap strap toward the center of the rotor; counterbalance with a similar device. Spin the device at 14,000 x g to concentrate to < 100 µL. Remove the assembled device from the centrifuge and separate the **Filter Device** from the collection tube. Transfer the filtrate

from the collection tube to a clean centrifuge tube (not provided). **Save the filtrate until the experiments are done.**

**D5.** Repeat **Step D4** once.

**D6.** Transfer the concentrated sample from the **Filter Device** to a 1.5 mL micro-centrifuge tube (use the pipetman to measure the approximate volume of the concentrated sample).

Work quickly

**D7.** Add 50-200  $\mu\text{L}$  of **Labeling Buffer** to the **Filter Device** to rinse (actual volume of **Labeling Buffer** added will depend upon the calculated total volume in **Step D9**). Stir it gently with a pipet tip, then transfer the entire contents to the 1.5 mL micro-centrifuge tube from **Step D6**.

**D8.** Repeat **Step D7** once.

**D9.** Add **Labeling Buffer** to make up the total volume of the sample to **640  $\pm$  10  $\mu\text{L}$** .

**Calculation 3 for Less Antibody (Ab):**

$$\text{Volume of Reduced Antibody in Step D9 } (\mu\text{L}) = \text{Ab in mg} \times 213.3$$

**D10.** Vortex the combined antibody sample for 30 seconds and then spin down.

## 6. MMAF Labeling (Step 2 in Scheme 1)

Items needed: [Mc-MMAF solution from step A3](#), [Hazardous Waste Bag \(CM03HZ1\)](#), [Antibody Solution from step D10](#).

**E1.** With personal protection equipment on, carefully open the centrifuge tube containing Mc-MMAF from **Step A3**.

**E2.** Transfer the entire solution (**110  $\mu\text{L}$**  total) to the centrifuge tube containing antibody from **Step D10**. When you add the Mc-MMAF solution, place the pipette tip inside the antibody solution and then dispense the Mc-MMAF slowly while swirling the pipette tip. **Dispose of the pipette tip and Mc-MMAF tube in the hazardous waste bag.**

**Calculation 4 for Less Antibody (Ab):**

$$\text{Volume of MMAF Solution to be Transferred in Step E2 } (\mu\text{L}) = \text{Ab in mg} \times 36.7$$

**Dispose of the remainder of the Mc-MMAF solution in the hazardous waste bag.**

**E3.** Cap the centrifuge tube. Mix at 25°C or RT for 1 h.

**Time-saving tip:** While waiting for the reaction to complete, you can move on to **Step F1** and equilibrate the column for purification.

## 7. Purification of Conjugate

Items needed: [Desalting Column](#), [Storage Buffer \(1x PBS\)](#), [2.0 mL Centrifuge Tube \(CM03CT3\)](#), [Hazardous Waste Bag \(CM03HZ1\)](#), [Antibody Solution from Step E3](#).

**F1.** In a chemical hood, securely attach the **Desalting Column** to a support stand, lab frame, or any support rod. Remove the top and bottom caps from the column and allow the excess liquid to flow through by gravity. Collect the liquid in a flask.

**F2.** Add 5 mL of **Storage Buffer** and allow the buffer to completely enter the gel bed by gravity flow.

**F3.** Repeat **Step F2** twice.

**F4.** Spin the Mc-MMAF-labeled antibody solution from **Step E3** before opening it. Add the entire antibody solution to the column. **Dispose of the centrifuge tube in the hazardous waste bag.**

**F5.** Add 250  $\mu\text{L}$  of **Storage Buffer** and allow the liquid to enter the gel bed completely (**Note:** this elution buffer does not contain any of your product, you can let it drain to the waste).

**Calculation 5 for Less Antibody (Ab):**

$$\text{Volume of Storage buffer in Step F5 } (\mu\text{L}) = 1000 - \text{Ab in mg} \times 250$$

**F6.** Place a 2 mL centrifuge tube under the column. Add 1.25 mL of **Storage Buffer** to the column. Collect the eluent by gravity and allow the buffer to enter the gel bed completely.

**Calculation 6 for Less Antibody (Ab):**

$$\text{Volume of Storage buffer in Step F6 } (\mu\text{L}) = 500 + \text{Ab in mg} \times 250$$

**F7.** Label the tube as your product. Store your conjugate at 4°C. **Dispose of the Desalting Column in the hazardous waste bag and seal the bag. Dispose of the waste following regulations appropriate for your area.**

### Conjugate is Ready for Your Experiment

- **Specifications of your product:** Mc-MMAF-labeled antibodies with an average drug-to-antibody ratio (DAR) of 3-4. A typical batch contains more than 90% conjugated products by size exclusion chromatography (SEC) with less than 10% unreacted antibody and is free of any unreacted drug. The approximate concentration of the ADC is 1.2 mg/mL in PBS buffer assuming 50% recovery. You can determine the concentration and estimated DAR of the ADC by UV/vis spectrophotometry (see Other Considerations).

## Other Considerations

### 1. Concentration Determination for IgG Antibody (Unlabeled)

The accuracy of the IgG amount is important for obtaining an optimized DAR in this protocol. The simplest assay method for determining IgG concentration in solution is to measure the absorbance of the IgG at 280 nm (UV range) ( $A_{1\text{ mg/mL}} = 1.4$ ).

If your antibody comes with a buffer that has no UV absorbance at 280 nm, you can measure the UV absorbance prior to starting an experiment.

$$\text{Concentration (mg/mL) of IgG} = \frac{(A_{280})}{1.4}$$

If your antibody comes with a buffer that has UV absorbance at 280 nm, you can determine the concentration in **step B11** after exchanging it with Reducing Buffer and assuming **95%** recovery of the IgG after buffer exchange. Reducing Buffer does not contain any substances that will interfere with the UV measurement at 280 nm. The total volume of Reducing Buffer added in **Step B10** can be estimated based on the initially estimated amount of antibody and will not affect the conjugation too much if the volume is off to some extent.

$$\text{Concentration (mg/mL) of Starting IgG} = \frac{(A_{280})}{1.4 \times 0.95}$$

After calculating the total amount, follow the calculations in **Steps B10, C3, D9, E2, F5, and F6** to obtain the correct volumes to be added in each step.

### 2. Concentration Determination for ADC

To determine the concentration of the ADC, dilute your conjugate from **Step F7** with 1x PBS buffer. Measure the UV absorbance of the conjugate at 280 nm ( $A_{280}$ ) using a UV spectrometer and calculate the concentration based on the following formula:

$$\text{Concentration } (\mu\text{M}) \text{ of the dilute sample} = \frac{(A_{280}) \times 4.7619}{L}$$

$$\text{Concentration (mg/mL) of the dilute sample} = \frac{(A_{280}) \times 0.7143}{L}$$

Where **L** is the UV cell path length (cm). If you are using a 1 cm UV cell, you can dilute the conjugate 4 times to obtain a good reading.

For a typical IgG with MW of 150,000, the molar extinction coefficient is  $210,000 \text{ M}^{-1}\text{cm}^{-1}$ .

### 3. MW Calculation for ADC

Calculation of the MW of the conjugate:

$$\text{MW(ADC)} = n \times 925 + 150000$$

Where **n** is the average molar ratio of MMAF per antibody. Use 3.0 if you do not have the hydrophobic interaction chromatography (HIC) profile of your conjugates.

#### 4. Drug-to-Antibody Ratio (DAR) and Characterization by UV

In this kit, the target DAR is 3-4. Depending on your antibody, you may achieve a lower DAR. Unfortunately, Mc-MMAF doesn't have a characteristic UV absorbance that allows easier calculation of DAR by UV. For DAR calculation and to check the homogeneity of the ADC, you can analyze it by hydrophobic interaction chromatography (HIC). If you do not have access to such a facility setup, you can send your sample to CellMosaic for analysis.

#### 5. Characterization of ADC by HIC HPLC

For ADCs prepared via a reduced thiol of the antibody, hydrophobic interaction chromatography (HIC) HPLC is used to calculate the DAR and the heterogeneity of the ADCs. The conjugates are separated based on hydrophobicity. Antibodies loaded with the same number of drugs (same DAR) will have similar hydrophobicity and be eluted as a single peak. For a typical Mc-MMAF ADC, multiple peaks represent various amounts of drug-loaded ADCs. You will find examples of HIC HPLC profiles of Mc-MMAF ADCs of various antibodies in the Appendix.

CellMosaic offers an HIC buffer set ([Product #: CM02025](#)) for our customers to use with any HIC column. The CM02025 product sheet contains all of the information and methodology needed to run an HIC HPLC analysis.

If you do not have access to an HPLC facility, you can send your sample to CellMosaic for analysis.

#### 6. Characterization of ADC by SEC HPLC

Mc-MMAF is very hydrophobic. This kit is designed to minimize the aggregation and precipitation issues generally seen with Mc-MMAF labeling. However, you may still notice some solid precipitate out or ADC aggregation during the reaction. The precipitate will be removed during purification. Depending on the properties of your antibody, recovery will be 40-80%. If you are concerned with the aggregation, you can use size exclusion chromatography (SEC) to check the extent of aggregation. SEC separates the conjugates by apparent molecular weight (MW) or size in aqueous solution. The larger the MW of the conjugate, the earlier it elutes. By comparing the SEC profile of unlabeled IgG and the ADC, you can estimate how much aggregation is in the ADC.

CellMosaic offers two SEC standards ([Product #: CM92004](#) and [CM92005](#)) for our customers to use with any SEC column. The CM92004 product sheet contains all of the information and methodology you need to run an SEC HPLC analysis.

If you do not have access to an HPLC facility, you can send your sample to CellMosaic for analysis.

#### 7. ADC Stabilizing Buffer

CellMosaic's proprietary ADC stabilizing PBS buffer (5x) ([Product #: CM02022](#)) contains 5x PBS buffer and other stabilizers to prevent the hydrophobic drugs from interacting with each other during storage, which would cause the ADCs to precipitate out. Stabilization buffer also helps preserve the structure of the ADCs during lyophilization. The buffer is biocompatible and can be

used directly for any *in vitro* and *in vivo* studies. For more information on the stabilization buffers, please check our website.

## 8. Recommended Storage Conditions

Recommend storage at 2-8°C for short-term. Do not freeze in PBS buffer. Based on our preliminary data, the conjugate made with this kit can remain stable in PBS buffer at 2-8 °C for few days. You may notice the increase amount of the aggregation after storing for sometimes. The stability of your conjugate may be different due to your antibody and should be checked either by HPLC or UV.

If you need to store the ADCs for long term, please dilute your ADC in Stabilization PBS buffer (5x) (included in this kit). Aliquot and store the conjugate in a < -20°C freezer or lyophilize to dryness. Avoid repeated freeze and thaw cycles. If the ADC is in a lyophilized powder, after dissolving, the solution should be used within few days.

## 9. Sample Submission for HPLC Analysis

If you are submitting samples to CellMosaic for SEC and HIC analysis, please follow these instructions:

- 1) Go online: <https://www.cellmosaic.com/hplc-analysis/>, select SEC HPLC Analysis ([Product# AS0023](#)) and HIC HPLC Analysis ([Product#: AS0025](#)), choose the quantity (number of samples. Bulk discounts available for multiple samples) and submit the order. Alternatively, you can email [info@cellmosaic.com](mailto:info@cellmosaic.com) for a quote and to place the order.
- 2) Dilute your un-conjugated antibody in PBS buffer to 1 mg/mL, and then transfer 50 µL of the diluted solution to a 500 µL micro-centrifuge tube. Label the vial properly.
- 3) Transfer 50 µL of ADC (non-diluted solution) to a 500 µL micro-centrifuge tube and label the vial properly.
- 4) Ship your samples with a cold pack for overnight delivery.


## Appendix: Typical Kit Performance Data (LC analysis, CellMosaic)

**Antibody information:** A therapeutic antibody (Human IgG1 subtype)


**Kit Lot number:** 5523.S12.021119

**Scale of the reaction:** 1 mg of antibody (protein content)

**Figure 1:** SEC HPLC analysis of purified Mc-MMAF-ADC.

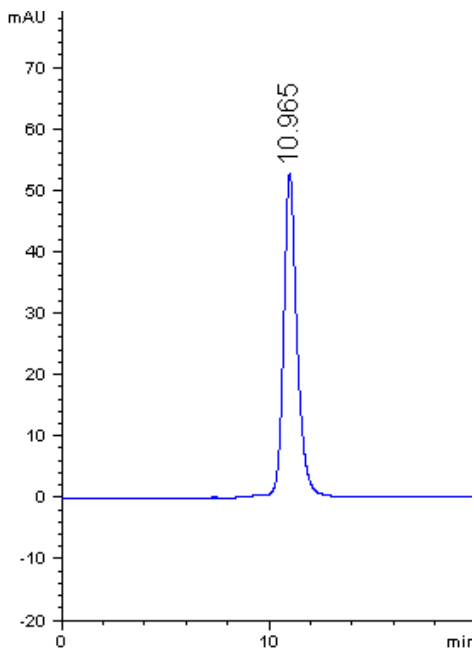

**Figure 2:** HIC HPLC analysis of antibody (red trace) and purified conjugates (blue trace)

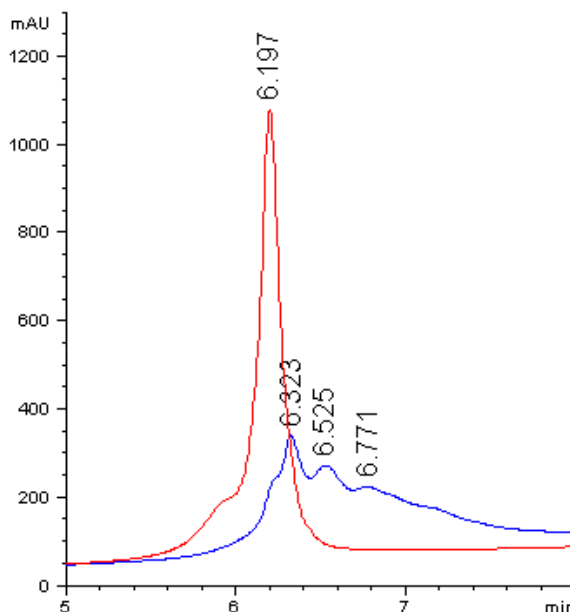

### Summary of the results:

Average DAR based on HIC HPLC	3
Extent of antibody aggregation (%)	0
Unreacted antibody (%)	0
Unreacted Mc-MMAF (%)	0
Recovery (%)	89