



CellMosaic, Inc.
10A Roessler Road
Woburn, MA 01801, USA
Phone: 781-463-0002; Fax: 781-998-4694; E-mail: info@cellmosaic.com

SEC (Gel filtration) HPLC Protein Standard

Each tube contains protein mixture lyophilized from 80 μ L of standard solution

Total 4 tubes

Product Number: **CM92004**

Product Description

CellMosaic's size exclusion chromatography (SEC) or gel filtration protein standard is designed for day to day use to check HPLC column performance and the analysis of bioconjugates. This product is a new formulation of our previously developed SEC protein standards (Part No. CM92002) and is a replacement for both SEC protein standards (Part No. CM92001 and CM92002). The new formulation allows the stable lyophilization of the protein mixture without changing its HPLC profile. The lyophilized protein mixture can be quickly reconstitution in water without any insoluble particles. The lyophilized product is also more stable for storage and can be shipped at RT.

The product consists of six proteins and one blue dextran with a MW range of 13.7 to 2000 KDa. The broad range of protein molecular weight coverage allows easy identification of small molecules, conjugates, and aggregates in a bioconjugation mixture, such as antibody-drug conjugation, protein, and antibody modification and conjugation. The product has been validated in many of the commonly used SEC columns. CellMosaic routinely uses this product for its internal bioconjugation-related research.

A total of four micro-centrifuge tubes are in a package. Each micro-centrifuge tube contains protein mixture lyophilized from 80 μ L of standard solution. The product is ready for use after reconstituting in 80 μ L of deionized water.

Application of the Product

- Calibration of gel filtration and size exclusion column
- Determination of the size and molecular mass of proteins
- Analysis of small molecules, bioconjugates, and aggregates

Key Features of the Product

- Lyophilized solid and ready to use for HPLC analysis after dissolving in water
- Mixture of 6 high purity proteins with broad MW coverage: 13.7 KDa to 2000 KDa

Composition

#	Name	MW (kDa)
1	RNase A	13.7
2	Carbonic anhydrase	29
3	Ovalbumin (albumin chicken egg)	43
4	Aldolase (rabbit muscle)	158
5	Ferritin (equine spleen)	440
6	Thyroglobulin	669
7	Blue dextran	2000

Storage/Stability

- Once reconstitute, CellMosaic's protein standard solution is stable at RT for months.
Recommended storage of the product is below -20°C, which is viable for several years without any sign of decomposition.

Procedure

1. Take one tube out and warm to ambient temperature.
2. Add 80 µL of deionized water and vortex for 30 seconds to dissolve.
3. Centrifuge briefly to ensure no liquid is in the cap. Transfer the supernatant to an HPLC vial.
4. Inject 8 µL for HPLC analysis (Note: the amount is optimized for a standard SEC HPLC analytical column with a volume of 10-15 mL. For lower or higher column volumes, scale the injection volume accordingly.)

Application Note

Calibration of Protein and Conjugate MW

The approximate MW of an unknown protein or protein conjugate can be determined by comparing its retention time to the protein standard. **Figure 1** gives an example of the SEC profile. For more accurate calculation, an SEC MW standard curve is recommended (**Figure 2**).

Figure 1. SEC HPLC profile of protein standards in a TSKgel BioAssist G3SW_{xl} (7.8 mm x 300 mm, 5 µm, Part No. 0008541). HPLC condition: isocratic PBS buffer at 0.5 mL/min. Instrument: Agilent 1100 HPLC series.

#	Name	MW (KDa)	Rt (min)
1	RNase A	13.7	21.397
2	Carbonic anhydrase	29	19.620
3	Ovalbumin (albumin chicken egg)	43	17.433
4	Aldolase (rabbit muscle)	158	15.923
5	Ferritin (equine spleen)	440	13.170
6	Thyroglobulin	669	11.562
7	Blue dextran	2000	11.099


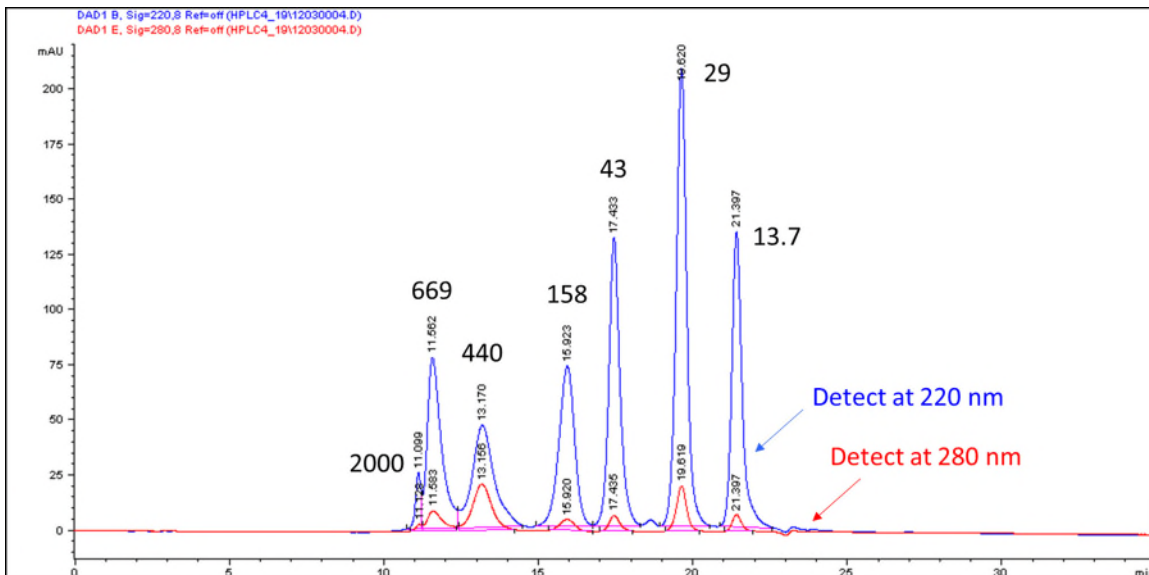


Figure 2. SEC MW standard curve of TSKgel BioAssist G3SW_{xl} (7.8 mm x 300 mm, Part No. 0008541). Data from Figure 1.

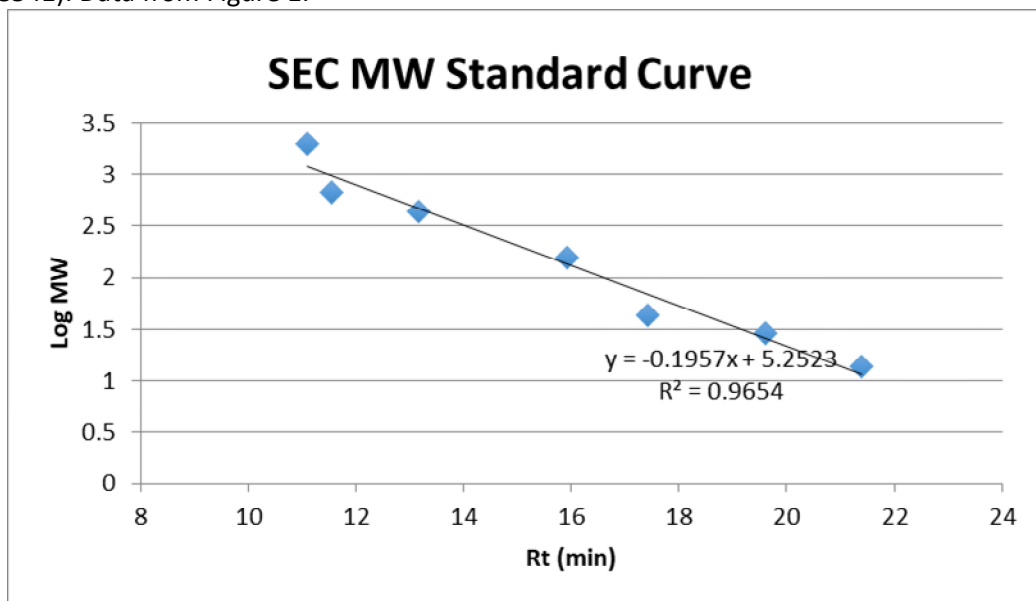

Assessing Column Performance

The protein standard mixture can be used to assess the column performance. The SEC profile of the protein standards may differ from column to column after some use. The quality of the SEC profile will indicate whether the column is good. For example, split peaks may indicate column resin-bound hydrophobic small molecules and that the column needs cleaning.

Important Notes & Contact Information

READ BEFORE USING ANY RESOURCES PROVIDED HEREIN

The information provided in this document and the methods included in this package are for information purposes only. CellMosaic provides no warranty of performance or suitability for the purpose described herein.

Sample data are provided for illustrative and example purposes only and represent a small dataset used to verify kit performance in the CellMosaic laboratory. Information about the chemicals and reagents used in the kit are provided as necessary.

For Research Use Only. Not for Use in Diagnostic Procedures.

The information in this document is subject to change without notice. CellMosaic assumes no responsibility for any errors that may appear in this document. In no event shall CellMosaic be liable, whether in contract, tort, warranty, or under any statute or on any other basis for special, incidental, indirect, punitive, multiple, or consequential damages in connection with or arising from this document, including but not limited to the use thereof.

NOTICE TO PURCHASER: LIMITED LICENSE

The purchase of this product includes a limited, non-transferable license to use this product to practice the labeling methods using the reagents solely for the purchaser's research activities. The license granted herein is personal to the original purchaser and may not be transferred to any other party outside the purchaser's company. No other right or license is conveyed or granted either expressly, by implication or by estoppel, to resell or repackage this product. Further information can be obtained by contacting:

Director of Licensing
c/o CellMosaic, Inc.
10-A Roessler Road, Woburn, MA 01801.
Phone: 781-463-0002
Fax: 781-998-4694
E-mail: info@cellmosaic.com